



# Mach LED 8MC Mach LED 6MC

Operating light system with LED technology



Operating light system with LED technology





Options:

Shadow Management

Camera Preparation

Laserpointer

Communication

Mechanical Adjustment (larger light field diameter)

Wall Operation

## Technical Data (1)

#### Mach LED 8MC light system

Light intensity at 1 meter distance

Colour temperature

Colour rendering index R<sub>a</sub>(2)

Colour rendering index R<sub>9</sub> (red) Focussable size of the light field

Working distance

Diameter of the lamphead

Temperature increase in the head area

Electronic light intensity control at the lamphead

Number of LEDs

Life-span of the LEDs

Total power consumption

#### Mach LED 8MC

70 - 160 cm

- Further technical details in the data sheet of the lamp, available upon request
  R<sub>a</sub> is an average of R<sub>1</sub> = burnt pink, R<sub>2</sub> = mustard yellow, R<sub>3</sub> = yellow green, R<sub>4</sub> = light green, R<sub>5</sub> = turquoise blue, R<sub>6</sub> = skyviolet, R<sub>7</sub> = violet, R<sub>8</sub> = lilac. Maximum value = 100.
  19 36 cm with the option mechanical adjustment



# Operating light system Mach LED 6MC

Operating light system with 140.000 lux (1 m distance) and electronic focussing

Options:

Shadow Management

Camera Preparation

Laserpointer

Communication

Mechanical Adjustment (larger light field diameter)

Wall Operation


Colour temperature Colour rendering index R<sub>a</sub>(2) Colour rendering index R<sub>9</sub> (red) Focussable size of the light field Working distance Diameter of the lamphead Electronic light intensity control at the lamphead Number of LEDs Life-span of the LEDs Total power consumption

# 70 - 160 cm 69 (66 with camera preparation) 60,000 h


- Further technical details in the data sheet of the lamp, available upon request
  R<sub>a</sub> is an average of R<sub>1</sub> = burnt pink, R<sub>2</sub> = mustard yellow, R<sub>3</sub> = yellow green, R<sub>4</sub> = light green, R<sub>5</sub> = turquoise blue, R<sub>6</sub> = skyviolet, R<sub>7</sub> = violet, R<sub>8</sub> = lilac. Maximum value = 100.
  18 34 cm with the option mechanical adjustment



# Mach LED 8MC / Mach LED 8MC

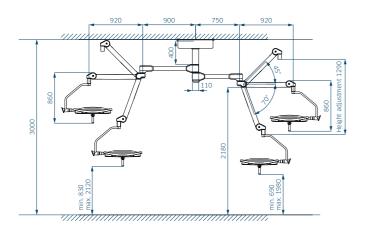


# Mach LED 6MC / Mach LED 6MC

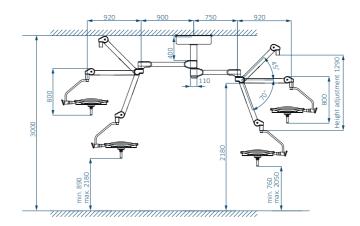




# Mach LED 8MC / Mach LED 6MC

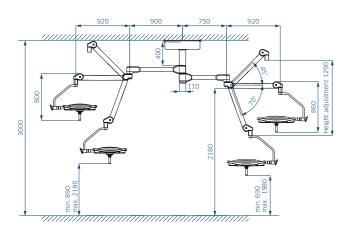

# Mach LED 8MC / Mach LED 6MC / Monitor

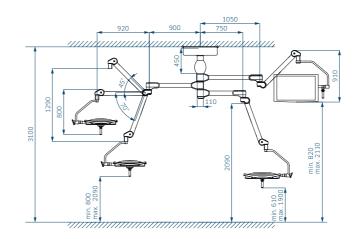



### Dr. Mach LED Technology


#### Close to perfect colour rendition

With colour rendering indexes  $R_a = 98$  and  $R_9$  (red) = 99 the surgeon recognizes clearly the tinies nuances of colour in tissue and thus a close to perfect image. For recognizing the exact colour spectrum of the wound the exact rendition of the red colour range is essential.  $R_9$  (red) = 99 means for the surgeon a visibly better recognition of details. The colour spectrum of the wound is rendered naturally with rich contrast. The OT-light clearly provides welcome relief for your eyes.



#### Antibacterial coating

To improve hygiene in the OR to a maximum, the operating lights of the new generation have a closed, easy-to-clean surface. In addition, they have an antimicrobial coating, which prevents the growth of microorganisms and thus helps to avoid infections.



One of the highlights of the new Mach LED 6MC and the new Mach LED 8MC is the cascade system. Different lens types are used in this system. These lenses have their focusing at 70, 100 and 130 cm. With this technology, a vertical focusing of the light beam throughout the depth of the wound canal can be achieved. As a result of this, it is no longer necessary for the surgeon to manually adjust the operation light field at the operating site.



# Ideal flow properties

During development high attention was paid to the performance of the new LED OT-lights in laminar-flow ceiling systems.


#### Large focussing range

The light field can be focused by turning the handle. The focussable light beam allows a punctual illumination of deepest wound channels with high intensity and an exact matching of the light field diameter with the size of the surgical requirements. The focusing is achieved by means of both a mechanical (optional) and electronical adjustment. The brightness of the light field remains constant.



#### Automatic shadow management

A further innovation is the shadow management, which is rendered possible by numerous sensors in the light. Any cluster that has its light disturbed by the surgeon is automatically turned off. At the same time, the other light clusters increase intensity in order to compensate for the shadow. Even with the surgeon continuously changing position, the light field remains homogeneously illuminated, without the need for manual adjustment of the light.

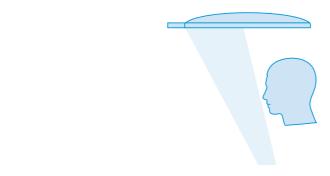

10 11

#### Dr. Mach GmbH & Co. KG

Flossmannstraße 28 85560 Ebersberg Germany

Phone: +49 (0) 8092 / 20 93-0 Fax: +49 (0) 8092 / 20 93-50 E-mail: info@dr-mach.de

